

ATP+AMP hygiene monitoring test

New Release


Lumitester™ PD-30 & LuciPac™ Pen

Invisible contaminants detected anywhere, anytime, by anybody in mere 10 seconds

Ultrahigh sensitivity attained with ATP plus AMP detection

US Patent No. 5891659

LuciPac Pen

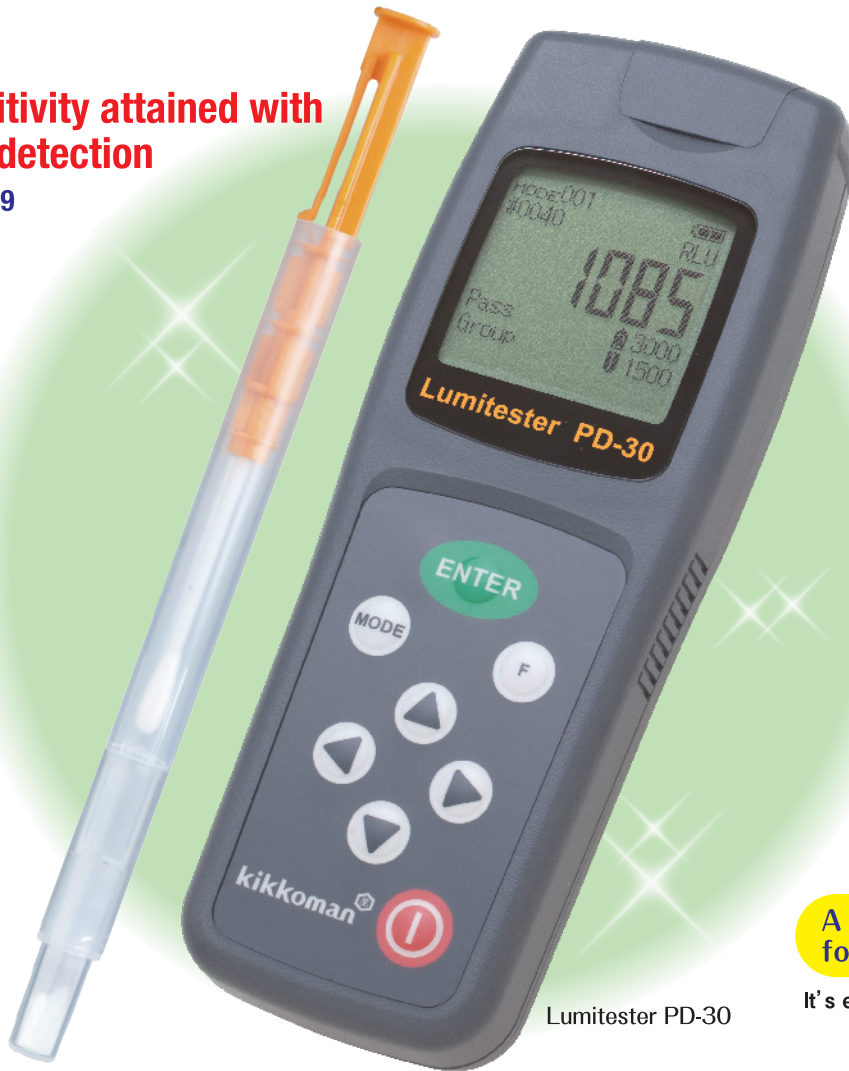

Lumitester PD-30



A soft case that allows for upright positioning.

It's easy to carry and resists soiling.

Enhanced new features at the comparable price as the previous model!

Temperature compensation


Select this function for stable measurements at 10-40°C.



8 Language Display Options

Select the display language from the eight languages provided. This facilitates the use of the Lumitester PD-30 overseas.



- English
- French
- Korean
- Chinese (both simplified and traditional)
- German
- Spanish
- Japanese



Data Analysis Software

The upgraded data analysis software allows you to match the testing mode to various measurement sites and situations.

MODE	Level 1	Level 2	Object
1	1500	3000	Worker A hands and
2	1500	3000	Worker B hands and
3	1500	3000	Worker C hands and
4	1500	3000	Worker D hands and
5	0500	1000	Refrigerator A han
6	0500	1000	Refrigerator B han
7	0500	1000	Refrigerator C han
8	0500	1000	Refrigerator D han
9	0500	1000	Doorknob A
10	0500	1000	Doorknob B
11	0500	1000	Doorknob C
12	0500	1000	Doorknob D
13	0500	1000	Faustel A handle
14	0500	1000	Faustel B handle
15	0500	1000	Faustel C handle



Lumitester PD-30



Lumitester PD-30

Self-diagnosis

Check cleanliness of the measurement chamber of the Lumitester PD-30.


Now you can ensure a clean environment and raise worker awareness of better hygiene. Work toward to permanently eliminate the risk of food poisoning with Lumitester.

- The ATP swab test is listed in the Guidelines on Food Hygiene Testing 2004 supervised by the Japanese Ministry of Health, Labor and Welfare.
- The ATP swab test is the first step toward attaining HACCP.

Restaurants and Institution Kitchens

Prevent secondary contamination with the most sanitary practices.

- Perform on-site and instant measurement of cleanliness conditions. If an unsafe cleanliness level is indicated, perform additional washing to prevent secondary contamination.
- A numerical display of test results allows effective cleanliness management, comparing readings from different shops, sites, etc.

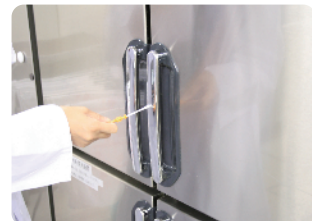

Food Processing Plants

Measure the cleanliness of your production sites.

- For effective and accurate checks after daily washings. In emergencies, pinpoint any contamination site rapidly.
- Thorough washing reduces the amount of residual allergens and contaminants.



Hygiene Education

Conduct effective hygiene education and training for employees and/or students at educational institutions.

- An instant readout display leaves no doubt of any contamination conditions. It also is good for educational/training purposes.



Easy Usage

- Wet the cotton swab with tap water (or distilled water if required) of the LuciPac Pen. Wipe the object/sample with the swab.
- Return the swab back into the swab holder of the LuciPac Pen. Lightly push the end of the swab holder and shake down the liquid stored midway in the LuciPac Pen. Shake well to thoroughly dissolve the powdered reagent.
- Measure the cleanliness indication by inserting the LuciPac Pen into the measurement chamber of Lumitester PD-30. Press "ENTER" key of the Lumitester PD-30 to start measurement.

Lumitester PD-30 (Product Code: 60486)	
Measurement Time	10 sec. (20 sec. when using temperature compensation in cold temperatures)
Measurement Temperature	10-40°C when temperature compensation function is ON 20-35°C when temperature compensation function is OFF
Data Output	Relative Light Unit (RLU)
Data Memory	2000 pcs of data
Power	Two AA alkaline or nickel hydride rechargeable batteries
Dimensions	65x175x32mm, approx. 235g (excl. batteries)
Accessories	Two AA alkaline batteries, cleaning brush, USB cable, strap, Quick Manual, CD-ROM, stand-up soft case

LuciPac Pen (Product Code: 60331)	
Appearance	An integrated testing device that containing the cotton swab, ATP releasing reagent, and luminescent reagent.
Packing	20 sticks in an aluminum packs; 5 packs make one kit (100 sticks/kit)
Material	Polypropylene
Storage	2-8°C (should not freeze) 14 days at 25°C (when pack has not been opened) 5 days at 30°C (when pack has not been opened)
Expiry	14 months after manufacture

※Use LuciPac Pen for Lumitester PD-20 or PD-30. Do not use it for other models.

※Readouts are the same as the older Lumitester models PD-10 (N) and PD-20.
※Do not use this product for purposes other than hygiene monitoring tests.
※Not to be used for counting general living bacteria or detecting specific pathogens.

Manufacture and Sales

kikkoman

Kikkoman Biochemifa Company

2-1-1 Nishi-Shinbashi, Minato-ku, Tokyo
105-0003 JAPAN
TEL:+81-3-5521-5490 FAX:+81-3-5521-5498
Email:Biochemifa@mail.kikkoman.co.jp
URL:http://biochemifa.kikkoman.co.jp/e

*Lumitester® and LuciPac® are registered trademarks of Kikkoman Corporation in Japan and other countries.
The information contained herein is subject to change without further notice.

©2014 Kikkoman Corp.(20140301)